

# Clinical Evaluation Data

## -Rodent Thyroid 3종



Item : Rodent Total T3


Lot : R3JE00

Sample : Abnova Rodent T3 ELISA Kit Calibrator

Comparison equipment : Abnova Rodent T4 ELISA Kit

Reference Range : 0.000 – 6.0 ng/mL

Sample No.	Expected Conc.	Result	CV (%)
1	0.00	0.01	-
2	0.25	0.37	17.7
3	0.50	0.47	5.2
4	1.00	1.21	4.0
5	2.50	2.50	4.2
6	5.00	5.08	2.7
7	7.50	7.60	2.9

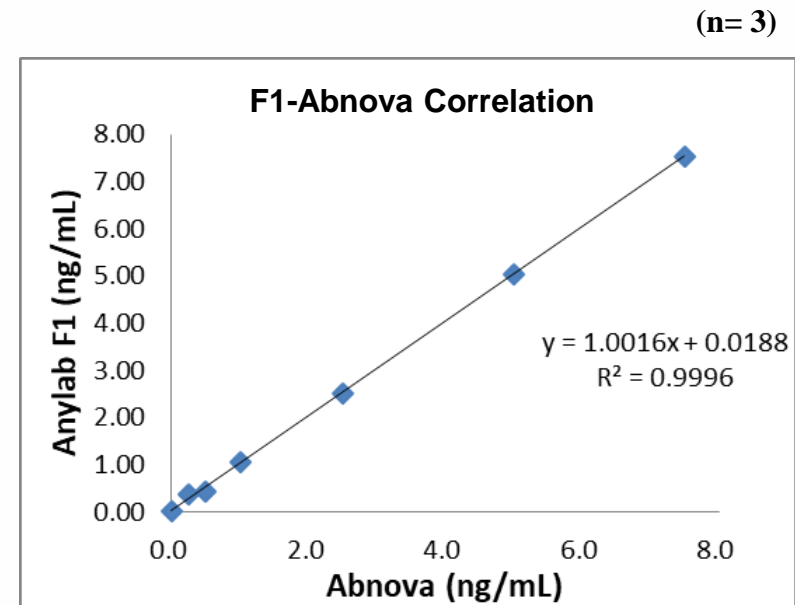



Item : Rodent Total T4


Lot : R4JE00

Sample : Abnova Rodent T4 ELISA Kit Calibrator

Comparison equipment : Abnova Rodent T4 ELISA Kit

Reference Range : 0.1 – 30.0 ug/dL

Sample No.	Expected Conc.	Result	CV (%)
1	0.0	0.10	4.8
2	0.5	0.31	3.9
3	1.0	0.79	2.0
4	2.5	2.42	2.4
5	5.0	4.82	0.9
6	10.0	9.96	1.3
7	30.00	29.88	2.1

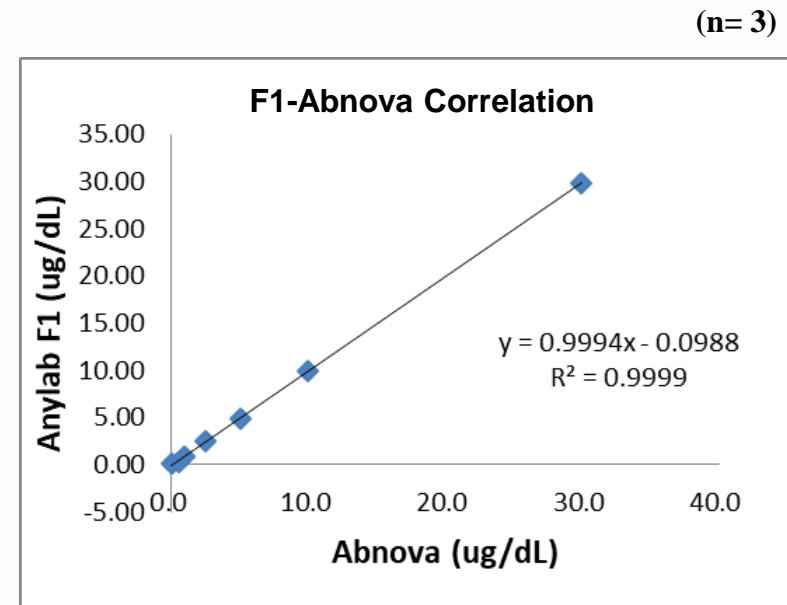



Item : Rodent TSH

Lot : RSJI01

Sample : Abnova Rodent TSH ELISA Kit Calibrator

Comparison equipment : Abnova Rodent TSH ELISA Kit

Reference Range : 0.000 – 100.000 ng/mL

Sample No.	Expected Conc.	Result	CV (%)
1	0.000	0.152	-
2	1.000	0.859	7.7
3	2.500	2.604	5.0
4	5.000	4.744	3.8
5	10.000	10.170	2.2
6	25.000	24.974	1.1

